

Fitting and Evaluating a Hearing Aid for Recipients of a Unilateral Cochlear Implant: The NAL Approach

Part 2. Bimodal hearing should be standard for most cochlear implant users

By Teresa YC Ching, PhD; Paula Incerti, MAud; Mandy Hill, DipAuD; and Jane Brew, MAud

Unless there is a clear indication that bimodal device use is counter-productive, bimodal stimulation should be the standard practice for clinical management of children and adults who receive unilateral cochlear implants and who have functional residual hearing in the non-implanted ear. Part 2 of this two-part article summarizes empirical evidence on the binaural benefits derived from wearing a hearing aid with a cochlear implant (bimodal hearing devices).

Editor's Note: Part 1 of this article, which appeared in last month's HR, described the NAL protocol for fitting a hearing aid on the opposite ear of a cochlear implant.

A person who has severe to profound hearing loss in both ears but wears a cochlear implant in only one ear may experience considerable hearing deficits in localization and speech intelligibility. The ability to localize sounds is highly dependent on being able to perceive sounds in both ears. When low frequencies are clearly audible in both ears, the brain can make use of the differences in time and intensity of sounds reaching the two ears to locate where a sound comes from on the horizontal plane. When sounds are inaudible in one ear, localization becomes very difficult.^{1,2} Reduced localization may lead to reduced safety, and difficulties in social functioning when understanding speech is reliant on lipreading.

Further, listening with two ears enables a person to understand more when speech occurs in background noise. This is because binaural processes related to head diffraction, binaural squelch, and binaural redundancy facilitate speech perception.³ Due to the physical size of the head, a sound on the right side of the head will

reach the right ear a bit sooner than it will reach the left ear. It will also be slightly louder in the right than in the left ear. This head diffraction effect will enhance speech intelligibility in noise when speech and noise come from different sides of the head, because the brain can selectively attend to the ear with a better signal-to-noise ratio (SNR) for understanding speech.

Even when the same signal and noise reach both ears, the brain can combine both inputs to produce more salient central representations of the speech signal (binaural redundancy) than if only input from one ear is available. The brain can also make use of the inter-aural time differences to partially reduce the deleterious effect of noise (binaural squelch).

For unilateral cochlear implant users who have residual hearing in the non-implanted ear, it is possible to provide binaural hearing by fitting a hearing aid to that ear. Increasing evidence points to the binaural benefits that are possible with the use of bimodal hearing devices, including improved speech intelligibility, better sound localization, and functional improvements in real-life environments. This article examines this research and discusses clinical issues related to bimodal device use.

Speech Intelligibility

Many studies have measured the speech perceptual abilities of people who use a cochlear implant and a hearing aid in the opposite ears. Although the studies differ in the speech material and test methods used, the results consistently show binaural benefits with bimodal hear-



Teresa YC Ching, PhD, (pictured) is senior research scientist and Mandy Hill, DipAuD, is a research audiologist research audiologists at the National Acoustics Laboratories (NAL) in Sydney, Australia. Paula Incerti, MAud, and Jane Brew, MAud, are research audiologists at the Sydney Cochlear Implant Centre.

ing. The following summarizes data of those that evaluated binaural redundancy, and others that assessed head diffraction effects and binaural squelch effects.

Binaural Redundancy. When speech and noise were presented from the same

loudspeaker positioned at a fixed distance in front of the subject, the SNR is similar at both ears. In this test situation, binaural/bimodal hearing is still superior to monaural hearing with cochlear implant alone (CI), as long as the hearing aid causes speech in any frequency range to be audible. Figures 1a-b summarize the sentence perception data reported in previous literature for adults⁴⁻¹¹ and for children.¹²⁻¹⁴ Results from listening in quiet (Figure 1a) and in noise (Figure 1b) are shown, with averaged results from each study represented by a data point. Greater binaural/bimodal advantage is evident for speech perception in noise than in quiet.

Head Diffraction. The effect of head diffraction has been measured by presenting speech and noise from spatially separated sources in two studies for adult listeners^{8,10} and one study for child listeners.¹⁴ Data on the mean cochlear implant (CI) and cochlear implant and hearing aid (CIHA) scores reported in these studies are shown in Figure 1c, with each data point representing averaged results from one study.

Both adults and children understood sentences better in noise when using CIHA compared to CI alone. These results were obtained when speech was presented nearer to the hearing aid side, and noise was presented nearer to the cochlear implant side. The hearing aid would, of course, not lead to any benefit (or may even be detrimental to speech perception), if speech were to come from the side nearer the cochlear implant and noise from the side nearer the hearing aid.⁸

Access to head diffraction differences is possible only if the hearing aid causes the mid- or high-frequency components of speech to be clearly audible. It follows that benefits due to head diffraction effects may be compromised when the residual hearing in the ear aided with a hearing aid is limited to very low frequencies, and when the hearing aid fitting does not provide adequate audibility at frequencies where there is functional hearing.

The speech results from both adults and children shown in Figure 1 support the fitting of a hearing aid to the non-implanted ear of unilateral cochlear implant

recipients when there is functional residual hearing in that ear.

Binaural Squelch. People who use current bimodal hearing devices are not able to make use of binaural squelch to enhance speech perception in noise. This is supported by direct research into the ability of hearing-impaired listeners to make use of inter-aural time delay for perceiving sentences in speech-shaped noise.¹⁵ The study concluded that *normal-hearing* listeners and *moderately hearing-impaired* listeners using bilateral hearing aids perceived sentences better when the noise was delayed in one ear relative to the other than when it was not delayed; however, the same was not observed for listeners with more *severe hearing losses*, irrespective of whether they used bilateral hearing aids or bimodal hearing devices.

This finding is consistent with a previous study on hearing-impaired listeners showing that the ability to use inter-aural time differences decreases as hearing loss increases, and that masking release is negligible for hearing losses exceeding 50 dB HL.¹⁶ Even if users of bimodal hearing devices have moderate degrees of hearing loss in the non-implanted ear, their access to binaural squelch will be limited by the extent to which the cochlear implant preserves fine timing information.

Localization Advantages

A few studies have examined the sound localization ability of children^{13,14,17} and adults^{8,10} who use unilateral cochlear implants. Measurement methods varied in detail, but such variations do not alter the two general findings: 1) Localization ability is poor for unilateral cochlear implant users, and 2) Localization ability is improved when a hearing aid is worn with a cochlear implant.

Figure 2 shows mean results summarized from the three studies on children and one study on adults that reported root mean square (rms) localization errors. (Note: Tyler et al.⁸ reports a percentage-correct score rather than rms error for 3 adults tested using an array of two loudspeakers.) The data on adults were drawn from Ching et al.¹⁰ in which an array of 11 loudspeakers (a 180° arc, with loudspeakers at 18° apart) were used and pink noise pulses were presented at 65 dB SPL from one of the loudspeakers at random. The subjects responded by identifying the loudspeaker from which the noise was emitted. Data

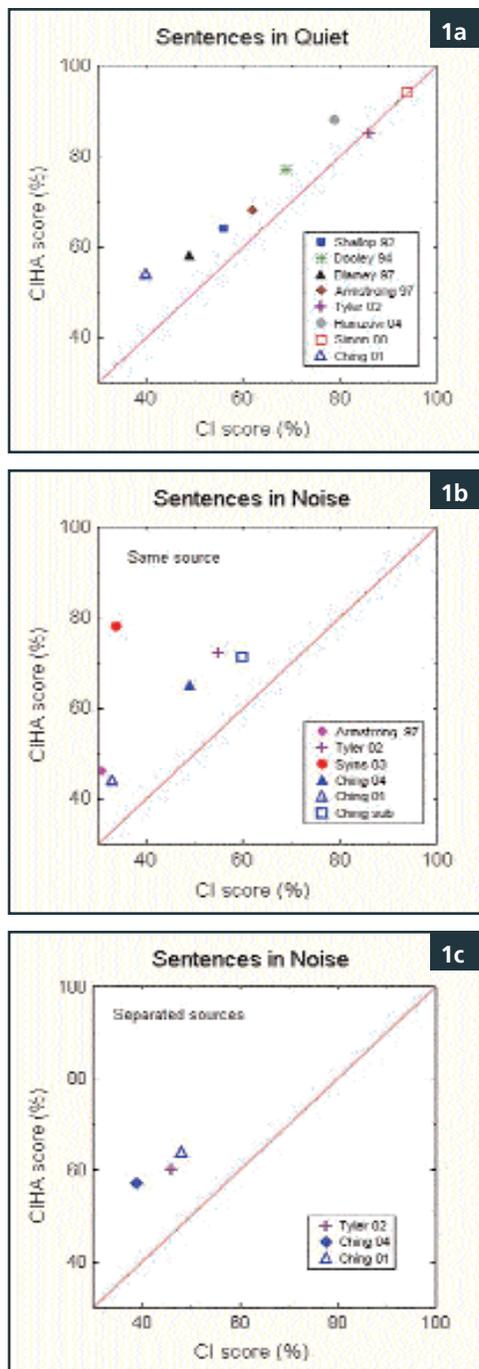


FIGURE 1. Sentence perception in quiet and in noise from spatially co-incident sources (1a and 1b), and sentence perception in noise from spatially separated sources (1c). Percent correct scores for cochlear implant alone (CI) are presented in relation to those for cochlear implant and hearing aid (CIHA). Each data point shows the averaged results from one study. The filled symbols are for adults and the open symbols are for children. The diagonal line represents no improvement of the CIHA condition over the CI condition. Improved performance with bimodal device use is shown by higher scores (ie, data points above the diagonal line).

from two of the studies on children used the same test method,^{13,17} and data from one study¹⁴ was based on an array of 5 loudspeakers at 30° apart. Performance was scored as rms error between the source and the response loudspeakers, expressed as degrees.

These empirical results show that binaural interaction occurs with an implant and a hearing aid, and that both children and adults are able to make use of bimodal hearing to improve their localization ability compared to the use of a cochlear implant alone.

Functional Performance in Everyday Life

Several studies have reported anecdotal comments from users of bimodal hearing devices about the superiority of wearing a cochlear implant with a hearing aid in everyday life, compared to the use of a cochlear implant alone. The comments from adults⁶⁻¹⁰ and children¹² or parents of children^{13,14,17,18} are summarized in Table 1. Adults' preference for using bimodal hearing devices appears to be dominated by the "naturalness" of music, quality of speech and environmental sounds, and "clarity" and "distinctiveness" of people's voices. Parents commented on the children's improved social functioning abilities when using bimodal hearing devices due to increased ease of communication and enhanced confidence. Both adults and children commented on increased directional hearing, sense of security, and of sounds being perceived in the "middle" rather than in one ear.

Four studies have used structured

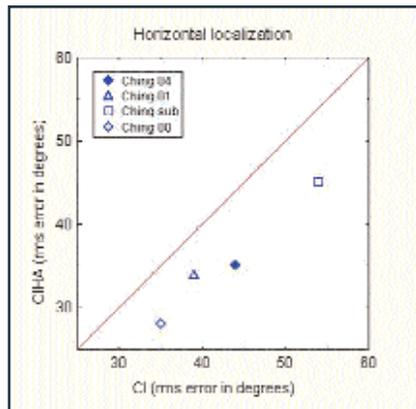


FIGURE 2. Horizontal localization with cochlear implant alone (CI) compared to cochlear implant with hearing aid (CIHA). Each data point represents averaged root mean square (rms) error score from one study, expressed in terms of azimuth degrees. The filled symbols are for adults, and the open symbols are for children. The diagonal line represents no improvement of the CIHA condition over the CI condition. Improved performance is shown by a reduction of errors (ie, data points below the diagonal line).

interviews based on questionnaires to solicit the information in a systematic way. The advantage in everyday life was quantified by comparing questionnaire

scores between the CIHA and the CI conditions, based on real-life experiences over a period of 1 week for each condition. Figure 3 summarizes the data from

STUDIES ON ADULTS		
Study	N	Bimodal advantages cited
Armstrong et al, 1997 ⁷	12	<ul style="list-style-type: none"> • more "natural" sound • sound is heard in both ears rather than through the implant alone • own voice quality is improved • a "full communication potential" is available
Blamey et al, 1997 ⁶	50	<ul style="list-style-type: none"> • hear sounds in both ears rather than on one side • "naturalness" of overall percept
Tyler et al, 2002 ⁸	3	<ul style="list-style-type: none"> • hearing aid picks up additional information, gives "clarified" hearing • feels more comfortable hearing sounds in both ears • gets more directional sound • hearing aid adds "a little/more" hearing level, while the cochlear implant "gives me the word and voice clarity."
Syms III & Wikesberg, 2003 ⁹	6	<ul style="list-style-type: none"> • better localization • better sound quality
Ching et al, 2004 ¹⁰	21	<ul style="list-style-type: none"> • adds more "brilliance" to people's voices • enjoy music more • easier to identify speaker in a group • easier to listen to speech in shops and restaurants • gives a "better balance" • more confident in everyday life
Hamzavi et al, 2004 ¹¹	7	<ul style="list-style-type: none"> • some directional hearing • more speech-like sound quality
STUDIES ON CHILDREN		
Simons-McCandless & Shelton, 2000 ¹²	4	<ul style="list-style-type: none"> • speech appears to be heard in the middle of his head rather than in one ear • provide added security if either were to stop working during a school day • prefers sound quality and localization ability with the use of both devices worn together
Ching et al, 2001 ¹³	11	<ul style="list-style-type: none"> • initiate more conversation • understand more of what's being said • require less repetition • more willing to converse with unfamiliar persons • more confident in shops
Ching et al, 2000 ¹⁷	5	<ul style="list-style-type: none"> • children generally functioned better in everyday life
Ching et al, 2002 ¹⁸	7	<ul style="list-style-type: none"> • picks up other people's conversation • speaks more clearly
Ching et al, 2004 (submitted) ¹⁴	18	<ul style="list-style-type: none"> • imitate voice and intonation better • can localize sounds better • more spontaneous and responsive in conversations • doesn't mishear as much • can recognize songs on the radio • can distinguish between environmental sounds • can distinguish between people's voices • more confident with friends • participates more actively in games • enjoys jokes more • more talkative • more attentive • less repetition required

TABLE 1. Summary of subjective comments of adults and children on the use of a cochlear implant with a hearing aid, compared to a cochlear implant alone.

adults¹⁰ and children,^{13,14,17} with the mean result from each study represented by a data point. Functional performance is better with CIHA than with CI alone, both for adults and for children.

In order to find out whether the children and adults who were fitted with a hearing aid due to their participation in a research study were wearing a hearing aid with a cochlear implant a year afterwards, we mailed out a questionnaire to all local participants (18 adults and 13 children) and conducted a telephone interview based on the questionnaire. The questionnaire included four questions on usage (How often did the subject use a cochlear implant and a hearing aid? A cochlear implant alone? Which was the preferred amplification mode? How much was the preferred mode better than the alternative mode?); and 12 questions on preferences in a range of specific situations (talking to family/friends in quiet; in transport; in noise; recognizing someone calling from behind and/or at a distance; watching TV or movie; and listening to music; localizing sounds; detecting/ recognizing sounds in the environment. For children, communication in the classroom and in the playground were included).

Of the 18 adults, 14 (78%) continued to use a hearing aid with an implant for at least 30 hours a week, two did not wear a hearing aid and were considering a second implant, and two had subsequently received a second cochlear implant. Of the 13 children, 10 (77%) continued to use a hearing aid with a cochlear implant. One child ceased wearing a hearing aid with a cochlear implant some time after her participation in the study, despite her indication that using bimodal hearing devices was “a lot better” than using a cochlear implant alone. This child was referred to her audiologist for follow-up counselling and management. One adolescent has not continued to wear a hearing aid now that he relies on his FM system that works with his implant only. One adolescent replied by mail because he could not communicate effectively over the phone. He uses a hearing aid alone, and doesn’t use his cochlear implant with his hearing aid because it aggravates the noise problem he encounters in his work environment.

Four adults and the parents of 12 children completed the entire questionnaire on rating the relative efficacy of bimodal hearing devices in a range of situations. Figure 4 shows the overall preference in relation to the preference averaged across specific

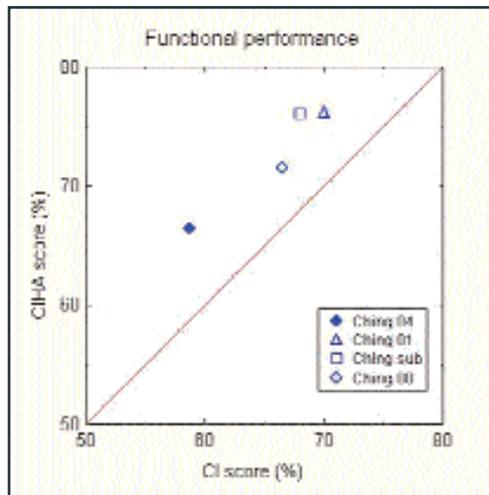


FIGURE 3. Functional performance with cochlear implant alone (CI) compared to cochlear implant with hearing aid (CIHA). Each data point represents averaged questionnaire scores in percentage terms. Results from children are based on parents’ questionnaire scores, and results from adults are based on the adults’ questionnaire scores. The diagonal line shows no improvement of the CIHA condition over the CI condition. Improved performance is shown by increased scores (ie, data points above the diagonal line).

situations. All except two children rated CIHA to be better than CI overall, and that rating was consistent with the ratings based on a range of situations in real life. The situations in which a hearing aid complements a cochlear implant most effectively for children are “talking to the teacher and to classmates in the classroom”; “talking to friends on the playground”; “recognizing the caller when he or she called from behind”; “communicating with family or friends in a bus/train/car”; and “localizing sounds”. One child commented especially on being able to hear better with both devices during dancing classes, and another commented on being able to hear the radio better when he used both devices.

All four of the adults who completed the questionnaire said that they continued to wear a hearing aid with a cochlear implant. Not only did they confirm that there were small improvements in understanding speech when “talking to family and friends in quiet and in noise” and “watching a movie or TV,” but they also attested to

the greater benefits associated with “listening to music”; “localizing sounds”; “recognizing sounds and voices in the environment”; and “recognizing who called when someone called from a distance and/or from behind.”

The adults also explained that they selectively used bimodal hearing devices in certain situations, but a cochlear implant alone in some other situations. For instance, one adult commented that she would turn her hearing aid off in noisy social situations when she wanted to listen to the friend on the side nearer her cochlear implant. Another commented that he would not wear his hearing aid when he rode his motorcycle so as to reduce wind noise.

These results from the follow-up study, albeit from a very small sample, confirmed the contribution of a contralateral hearing aid to a unilateral cochlear implant in some everyday life situations, but also revealed that individual management strategies are required to encourage the effective use of binaural amplification, especially for children.

Clinical Issues

Pre-implant and post-implant counseling. There is no direct evidence to indicate that people who received pre-implant counseling on the use of bimodal hearing are more likely to continue using

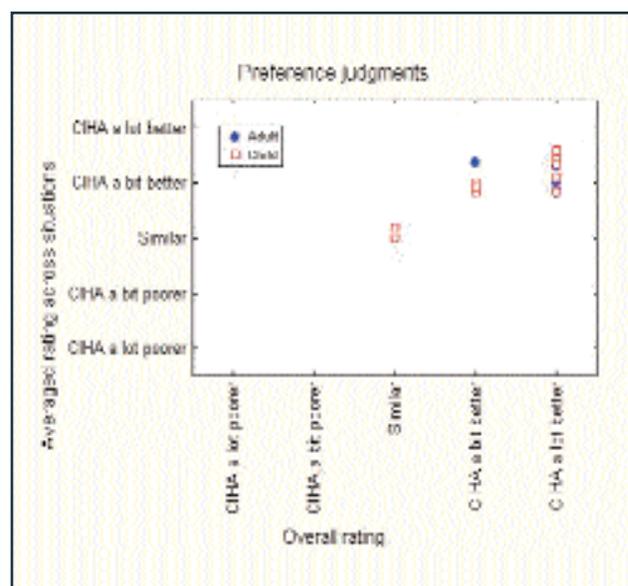


FIGURE 4. The overall preference rating in relation to the ratings averaged across 12 specific everyday life situations for adults (filled symbols) and children (open symbols).

a hearing aid after implantation. Indeed, a survey of 71 adults who received unilateral cochlear implants at the Melbourne implant clinic¹⁹ revealed that 53 (75%) continued to use a hearing aid in the non-implanted ear immediately after implantation although no specific counseling on bimodal hearing was provided. They rated bimodal hearing for speech in noise and localization to be significantly better than using a cochlear implant alone. Of the 53 adults, 51% had their hearing aids fine-

tuned to facilitate bimodal hearing. It is surmised that the remaining 26 users may derive greater binaural benefits if their hearing aids were fine-tuned with their cochlear implants.

For children, clinicians customarily discouraged hearing aid use after implantation.¹² Fortunately, this practice is changing as an increasing number of children who receive unilateral cochlear implants have functional residual hearing in the non-implanted ear, and evidence is

accumulating to indicate that the contralateral hearing aid complements the cochlear implant. Although there is no systematic data on the role of counseling, experience in practical management of children at the Sydney Cochlear Implant Centre supports the value of counseling for parents, teachers, and children (if applicable), and the implementation of individual management strategies in facilitating the use of a hearing aid with a cochlear implant for children.²⁰

Hearing aid fitting and fine-tuning. We recommend selecting a hearing aid using the NAL-RP prescription, in keeping with the empirical evidence showing that the prescription is appropriate on average (see Part 1 of this article in the July *HR*)²¹ Individual fine-tuning can be carried out 2-4 weeks after fitting using a systematic procedure to check that the hearing aid frequency response is best for speech intelligibility, and that the gain for low-level inputs and high-level inputs (or compression ratio) of the hearing aid provide a loudness sensation that is similar to that provided by the cochlear implant (ie, NAL approach described in Part 1). If an individual requires modifications in frequency response and/or gain, the procedure gives clear indications of how changes need to be made. Balancing the loudness between ears is essential for listening comfort, and could make the difference of a child using a hearing aid or not.

FM system. When a binaural FM system with independently adjustable gain for each ear is fitted to a child user of bimodal hearing devices, the child would not be expected to gain any advantages from head diffraction or binaural squelch in those circumstances where the FM system is actually used. However, the child would be able to derive the advantage arising from binaural redundancy.

Auditory experience. A clinical question remained as to whether one should fit a hearing aid to a child or adult who did not continue to wear a hearing aid after receiving a unilateral cochlear implant for some years. Previous evidence on bimodal hearing benefits have mostly been based on results from subjects that habitually used a hearing aid with a cochlear implant, with some suggestion that people who did not habitually use bimodal hearing derived less benefit.⁷

In contrast, recent research that compared the performance of adults and children who habitually wore a hearing aid

continued on page 63

with a cochlear implant to those who did not^{10,14} provide evidence that binaural benefits are possible for both groups of subjects after a short period of familiarization with the two devices. The results clearly indicated that both groups derived binaural benefits from bimodal hearing compared to using a cochlear implant alone. We therefore recommend fitting a hearing aid to the non-implanted ear of children or adults who discontinued hearing-aid use after implantation and who have functional residual hearing in that ear. Fine-tuning of the hearing aid can be carried out after about 4 weeks of familiarization with the use of a cochlear implant with a hearing aid.²¹

Possible disadvantages. Notwithstanding the accumulating evidence in support of the use of bimodal hearing devices, there may be some people who have deficits in binaural processing such that better performance is obtained with a unilateral device than with bilateral devices (indeed, this phenomenon has been observed for hearing aid wearers²²). Evidence for withdrawing hearing aid amplification for a unilateral cochlear implant recipient would include consistent and prolonged rejection of the hearing aid after the clinician has made every effort to fine-tune the fitting, as well as poorer speech test results when using bimodal hearing than when using a cochlear implant alone. For young children, parental reports based on systematic evaluation showing that the child functions better with a cochlear implant alone than with both devices during trial periods of a few days with the implant alone would also constitute evidence for withdrawal of the hearing aid.

Bimodal Hearing Should Be Standard for Most CI Users

Binaural processes operate only when sounds are audible in both ears, and research clearly shows that binaural processes contribute to benefits in speech intelligibility, localization, and functional performance of people who use bimodal hearing devices. Fitting a hearing aid to a recipient of a unilateral cochlear implant can help to improve the quality of life of the recipient and family. Wearing a hearing aid also eliminates the negative impact of auditory deprivation in the non-implanted ear. Other tangible advantages arising from the use of bimodal hearing devices include having access to directional microphones in both ears that will enhance speech perception in

noise,²³ enhanced sound quality,^{10,12,24} and having one device available when the other is not.

Unless there is a clear indication that bimodal device use is counter-productive, bimodal stimulation should be the *standard practice* for clinical management of children and adults who receive a unilateral cochlear implant and who have functional residual hearing in the non-implanted ear. ▀

References

1. Byrne D, Noble W, LePage B. Effects of long-term bilateral and unilateral fitting of different hearing aid types on the ability to locate sounds. *J Am Acad Audiol.* 1992;3:369-382.
2. Byrne D, Noble W. Optimizing sound localization with hearing aids. *Trends Amplif.* 1998;3(2):51-73.
3. Dillon H: *Hearing Aids.* New York City: Thieme; 2001.
4. Shallop JK, Arndt PL, Turnacliiff KA. Expanded indications for cochlear implantation: perceptual results in seven adults with residual hearing. *J Sp Lang Path Audiol.* 1992;16:141-148.
5. Dooley GJ, Blamey PJ, Seligman PM, Alcantara JI, Clark GM, Shallop JK, Arndt P, Heller JW, Menapace CM. Combined electrical and acoustical stimulation using a bimodal prosthesis. *Arch Otolaryng Head Neck Surg.* 1993;119:55-60.
6. Blamey P, Armstrong M, James C. Cochlear implants, hearing aids, or both together? In: GM Clark, ed. *Cochlear Implants.* Bologna, Italy: Monduzzi Editore; 273-277.
7. Armstrong M, Peg P, James C, Blamey P. Speech perception in noise with implant and hearing aid. *Am J Otol.* 1997;18:S140-S141.
8. Tyler RS, Parkinson AJ, Wilson BS, Witt S, Preece JP, Noble W. Patients utilizing a hearing aid and a cochlear implant: speech perception and localization. *Ear Hear.* 2002;23:98-105.
9. Syms III CA, Wickesberg J. Concurrent use of cochlear implants and hearing aids. In: Kubo T, Takahashi Y, Iwaki T, eds. *Cochlear Implants;* The Hague, The Netherlands: Kugler Publ; 2001.
10. Ching TYC, Incerti P, Hill M. Binaural benefits for adults who use hearing aids and cochlear implants in opposite ears. *Ear Hear.* 2004;25:9-21.
11. Hamzavi J, Pok SM, Gstoettner W, Baumgartner W-D. Speech perception with a cochlear implant used in conjunction with a hearing aid in the opposite ear. *Int J Audiol.* 2004;43:61-65.
12. Simons-McCandless M, Shelton C. Cochlear implants and hearing instruments: do they mix? *Hearing Review.* 2000;Nov:38-48.
13. Ching TYC, Psarros C, Hill M, Dillon H,

Incerti P. Should children who use cochlear implants wear hearing aids in the opposite ear? *Ear Hear.* 2001;22:365-380

14. Ching TYC, Hill M, Brew J, Incerti P, Priolo S, Rushbrook E, Forsythe L. The effect of auditory experience on speech perception, localization, and functional performance of children who use cochlear implants and hearing aids in opposite ears. *Int J Audiol.*, submitted.
15. Ching TYC, Hill M, van Wanrooy E, Dillon H. *Binaural intelligibility level differences for children and adults who use cochlear implants and hearing aids in opposite ears.* Poster presented at the CIAP Conference: Asilomar, Calif; 2003.
16. Jerger J, Brown D, Smith S. Effect of peripheral hearing loss on the MLD. *Arch Otolaryngol.* 1984;110:290-296.
17. Ching TYC, Psarros C, Hill M. Hearing aid use with the Nucleus 24 cochlear implant system for children who switched from the SPEAK to the ACE strategy. *Austral NZ J Audiol.* 2000; 22: 123-132.
18. Ching TYC, Psarros C, Hill M, Smither J: Should children who wear a cochlear implant in one ear use a hearing aid in the opposite ear? In: Seewald RC, Gravel JS, eds. *Proceedings of the Second International Conference: A Sound Foundation through Early Amplification 2001:* Warrenville, Ill: Phonak Inc; 2002:195-202.
19. Cowan R, Chin-Lenn J. "Bimodal hearing aid use" - Using a cochlear implant and hearing aid effectively. Paper presented at the 4th APSCI 2003: Taipei, Taiwan; 2003.
20. Ching TYC, Psarros C, Incerti P, Hill M. Management of children using cochlear implants and hearing aids. *Volta Rev.* 2003; 103(1):39-57.
21. Ching TYC, Hill M, Dillon H, van Wanrooy E. Fitting and evaluating a hearing aid for recipients of a unilateral cochlear implant: The NAL approach. *Hearing Review.* 2004;11(7):14-22,58.
22. Jerger J, Silman S, Lew H, Chmiel R. Case studies in binaural interference: converging evidence from behavioural and electrophysiologic measures. *J Am Acad Audiol.* 1993;4(2):122-131.
23. Ricketts TA. Directional hearing aids. *Trends Amplif.* 2001;5:139-176.
24. Balfour P, Hawkins D. A comparison of sound quality judgments for monaural and binaural hearing aid processed stimuli. *Ear Hear.* 1992;13(5):331-339.

Correspondence can be addressed to HR or Teresa YC Ching, PhD, National Acoustic Laboratories, 126 Greville St, Chatswood, NSW 2067, Australia; email: Teresa.Ching@nal.gov.au.